


Clinician guide: Real-time physiological monitoring


Prompting a patient to connect their monitoring device during a Video Call

Please note: the screenshots below serve as a guide and may differ slightly depending on your device or screen orientation (these screenshots are from a computer).

1. To enable your patient to pair their physiological monitoring device via Bluetooth, click on **Apps and Tools** at bottom right of the call screen.

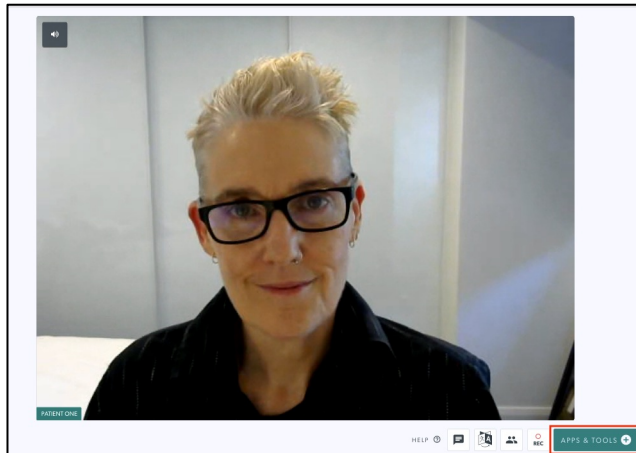

2. Next, select **Patient Monitoring Device** from the list of apps on the right hand side of your screen.

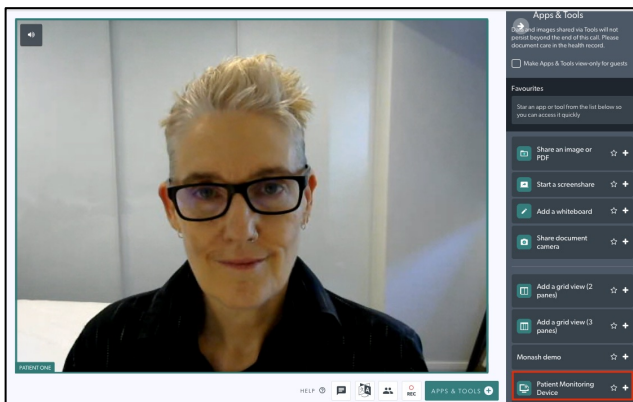


3. Instruct your patient to turn on their device and place it on their finger. Please note: your screen is a representation of the screen presented to your patient. Ask them to click on **Click Here to connect to your medical device**.



4. A popup will appear on the patient's screen, allowing them to select their monitoring device to **pair** it to the Video Call.


5. Your patient's readings should display on the screen after a few moments.

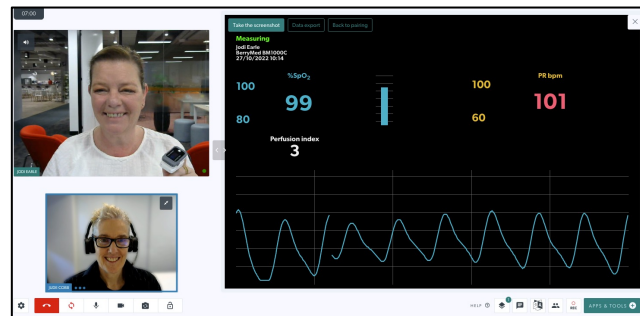


6. In the top left corner of the results screen, you have the following options:
 - **Take the screenshot** of the results;
 - Review the patient's data by selecting **Data export** in the top left corner. These results will download as a csv file.




7. If connectivity is lost, or readings are interrupted, you can select **Back to pairing** and prompt your patient to re-connect their device.

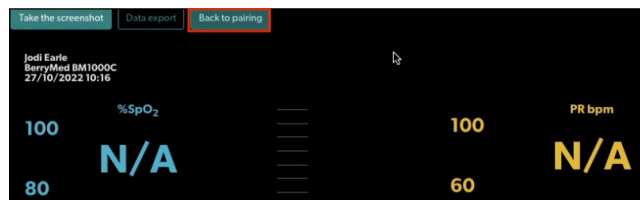

8. If Bluetooth pairing fails, instruct the patient to select **Add Manual Entry** instead. When entered correctly, their results will display as shown below.

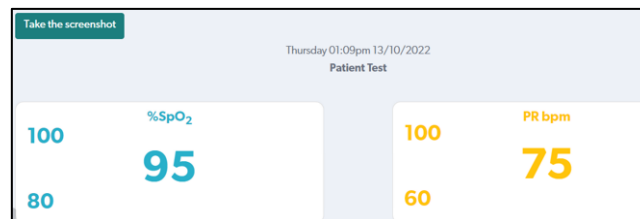

9. When the necessary readings have been reviewed or saved, you may exit the app by simply clicking on the X at top right, or on the **bin** icon to remove it from the Active Tools list.

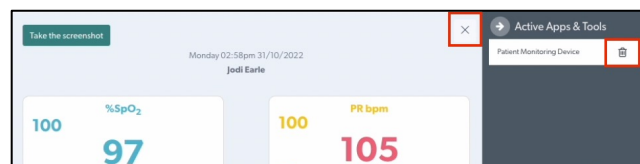

Use the link below or scan the QR code to access more information and support videos
help.vcc.healthdirect.org.au/remote-patient-monitoring

